


PRODUCT

VTS 256 PHARMACY REFRIGERATOR

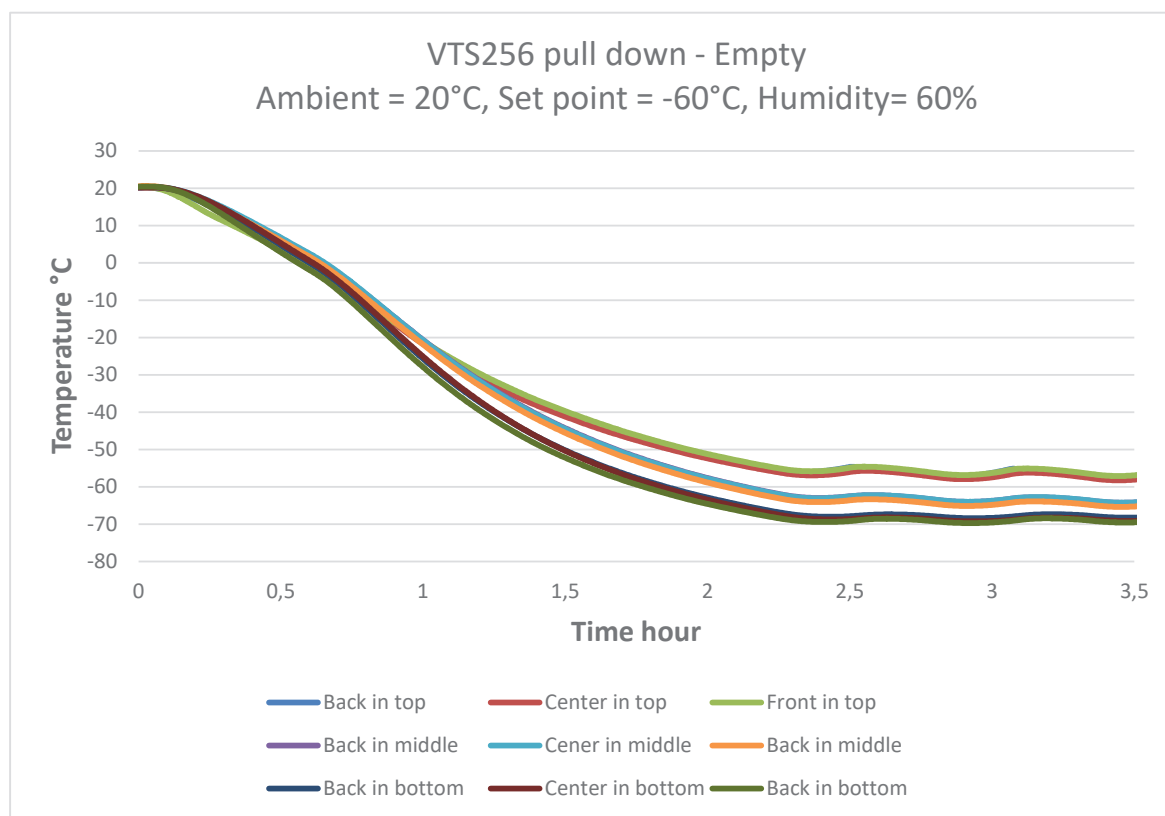

VESTFROST
SOLUTIONS

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.



BIOMEDICAL SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

Pull down test from ambient temperature – VTS 256

Test Conditions:

Model:	VTS 256
SN:	71769208
Test environment:	Controlled conditions
Ambient temperature:	+20°C ± 1°C
Ambient humidity:	60% ± 5%
Temperature set-point in cabinet:	-60°C
Cabinet load:	None
Door openings:	None
Sensors used:	25g tinned brass formed as a cylinder with diameter of 15.2mm
Sensors position:	9 points measure distributed diagonal in the cabinet layers. Sensors are placed with one in front where the door opens, one in the middle and one in the back opposite of the front sensor
Installation:	Appliance installed according to the instruction manual condition
Refrigerant:	Nature R

Result of test:

Starting at ambient temperature, the set point was reached after 140min.

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.




BIOMEDICAL SOLUTIONS

VESTFROST
SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

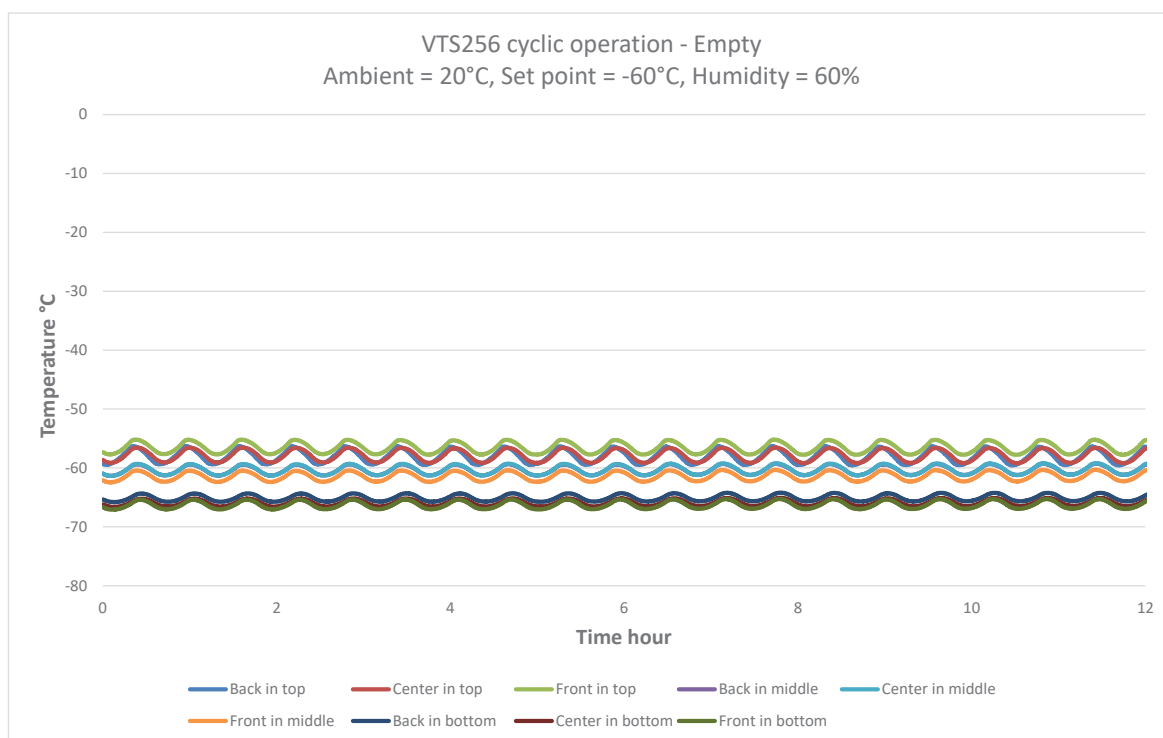

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.



BIOMEDICAL SOLUTIONS

VESTFROST
SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

Cyclic operation – VTS 256

Test Conditions:

Model:	VTS 256
SN:	71769208
Test environment:	Controlled conditions
Ambient temperatur:	+20°C ± 1°C
Ambient humidity:	60% ± 5%
Temperature set-point in cabinet:	-60°C
Cabinet load:	None
Door openings:	None
Sensors used:	25g tinned brass formed as a cylinder with diameter of 15.2mm
Sensors position:	9 points measure distributed diagonal in the cabinet layers. Sensors a placed with one in front where the door opens, one in the middle and one in the back opposite of the front sensor
Installation:	Appliance installed according to the instruction manual condition
Refrigerant:	Nature R

Result of test:

At an ambient temperature at 20°C, the energy for 24 hour is 6,108 kWh.

The temperature difference between top and bottom is 3,3°C

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.




BIOMEDICAL SOLUTIONS

VESTFROST
SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

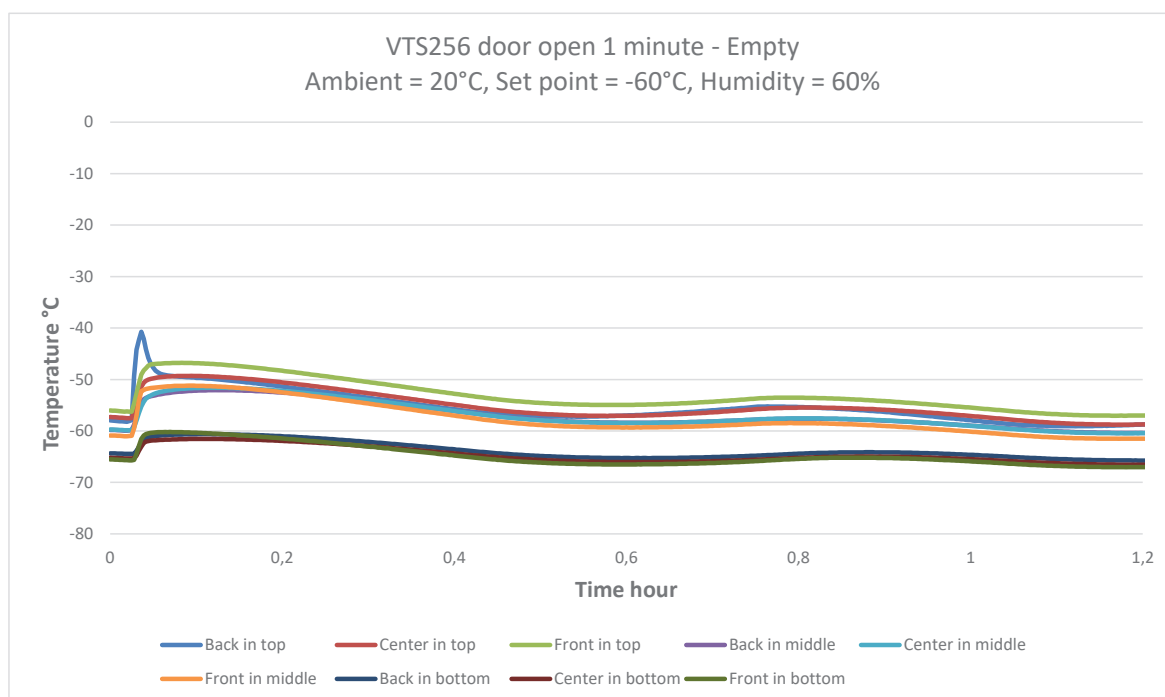

VESTFROST
SOLUTIONS

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.



BIOMEDICAL SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

Door open 1 minute – VTS 256

Test Conditions:

Model:	VTS 256
SN:	71769208
Test environment:	Controlled conditions
Ambient temperatur:	+20°C ± 1°C
Ambient humidity:	60% ± 5%
Temperature set-point in cabinet:	-60 °C
Cabinet load:	None
Door openings:	1 in 1 minute
Sensors used:	25g tinned brass formed as a cylinder with diameter of 15.2mm
Sensors position:	9 points measure distributed diagonal in the cabinet layers. Sensors a placed with one in front where the door opens, one in the middle and one in the back opposite of the front sensor
Installation:	Appliance installed according to the instruction manual condition
Refrigerant:	Nature R

Result of test:

Starting at set point, after a door opening of 1 minute, the temperature recovered to set point after 36 min

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.




BIOMEDICAL SOLUTIONS

VESTFROST
SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

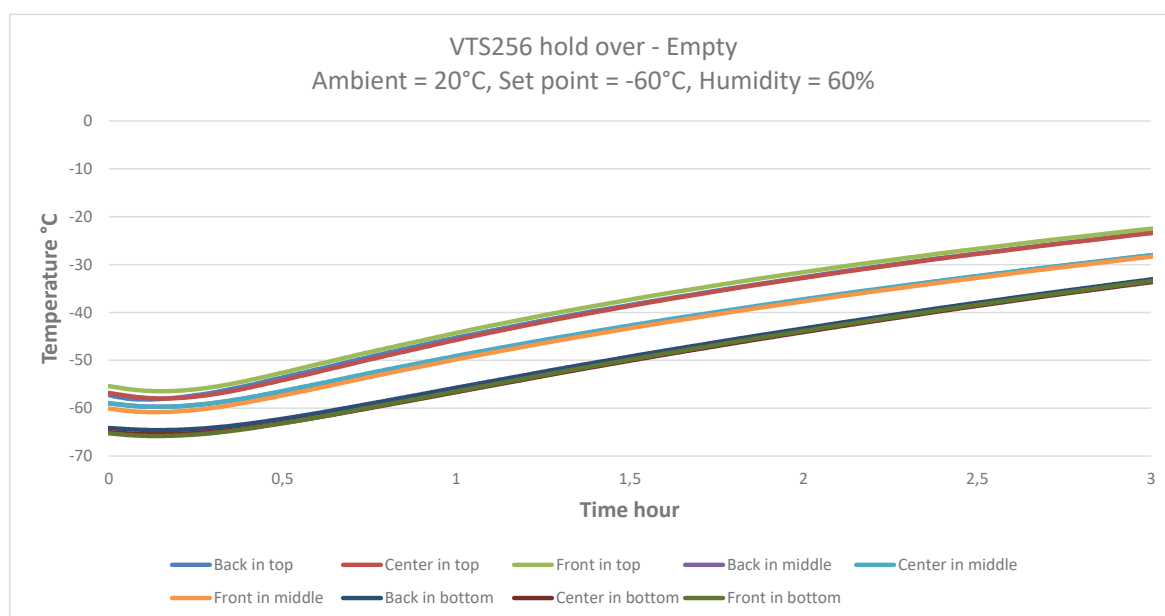

VESTFROST
SOLUTIONS

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.



BIOMEDICAL SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

Hold over time from -60°C to -40°C – VTS 256

Test Conditions:

Model:	VTS 256
SN:	71769208
Test environment:	Controlled conditions
Ambient temperature:	+20°C ± 1°C
Ambient humidity:	60% ± 5%
Temperature set-point in cabinet:	-60°C
Cabinet load:	None
Door openings:	None
Sensors used:	25g tinned brass formed as a cylinder with diameter of 15.2mm
Sensors position:	9 points measure distributed diagonal in the cabinet layers. Sensors are placed with one in front where the door opens, one in the middle and one in the back opposite of the front sensor
Installation:	Appliance installed according to the instruction manual condition
Refrigerant:	Nature R

Result of test:

Starting at set point temperature, the temperature rise above -40°C between 78min and 140min.

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.




BIOMEDICAL SOLUTIONS

VESTFROST
SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

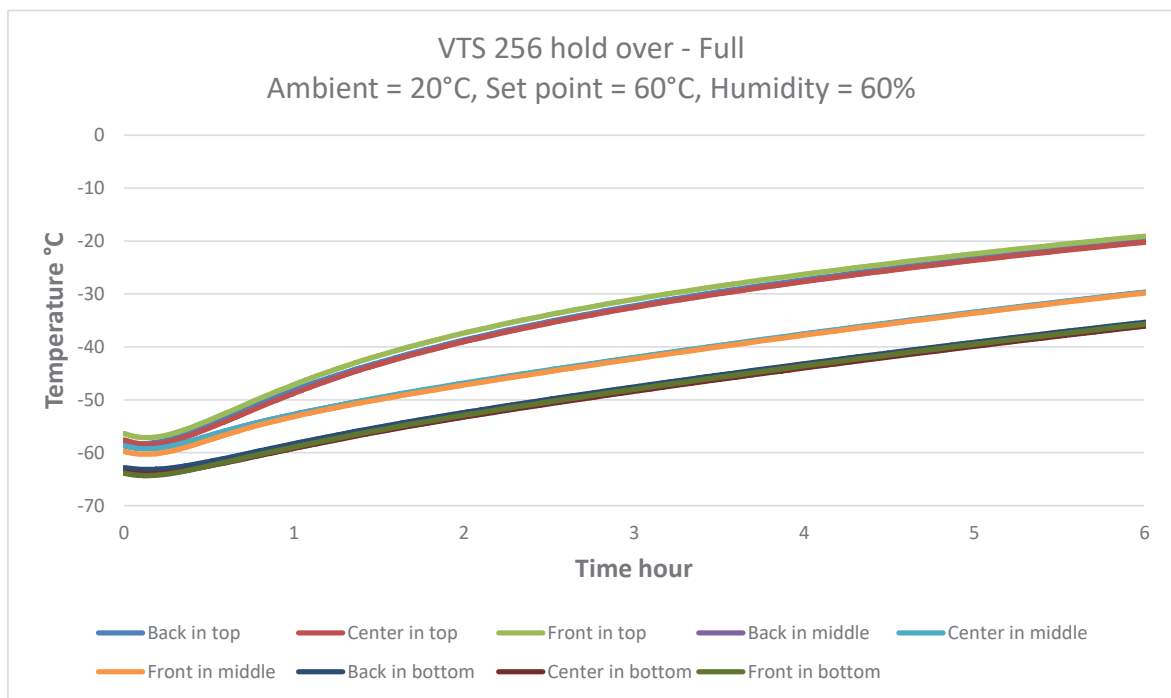

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.



BIOMEDICAL SOLUTIONS

VESTFROST
SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com

PRODUCT

VTS 256 PHARMACY REFRIGERATOR

Hold over time from -60°C to -40°C – VTS 256

Test Conditions:

Model:	VTS 256
SN:	71769208
Test environment:	Controlled conditions
Ambient temperature:	+20°C ± 1°C
Ambient humidity:	60% ± 5%
Temperature set-point in cabinet:	-60°C
Cabinet load:	Full
Door openings:	None
Sensors used:	25g tinned brass formed as a cylinder with diameter of 15.2mm
Sensors position:	9 points measure distributed diagonal in the cabinet layers. Sensors are placed with one in front where the door opens, one in the middle and one in the back opposite of the front sensor
Installation:	Appliance installed according to the instruction manual condition
Refrigerant:	Nature R

Result of test:

Starting at set point temperature, the temperature rise above -40°C between 102min and 290min.

Products are subject to change due to enhancements and continuous development. Vestfrost Solutions reserve the right to alter any information, without further notice.



BIOMEDICAL SOLUTIONS

VESTFROST
SOLUTIONS

A/S Vestfrost
Falkevej 12
DK-6705 Esbjerg Ø
www.vestfrostsolutions.com